





WARNING:
 THIS ILLUSTRATION DOES NOT NECESSARILY
 REFLECT THE ACTUAL CABLE CONFIGURATION.
 PLEASE REFER TO THE
 RESPECTIVE DATASHEET 1041.2421.51



AUXILIARY VIEW A
 SCALE 20 : 1
 LATERAL VIEW CLOSED WITH NO CABLES
 FOR ILLUSTRATION PURPOSES ONLY

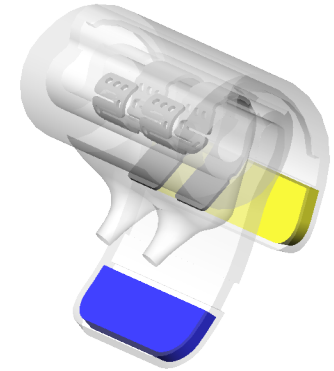

CLOSED CUFF 3D VIEW B
 SCALE 20 : 1
 CABLES NOT DISPLAYED
 FOR ILLUSTRATION PURPOSES ONLY

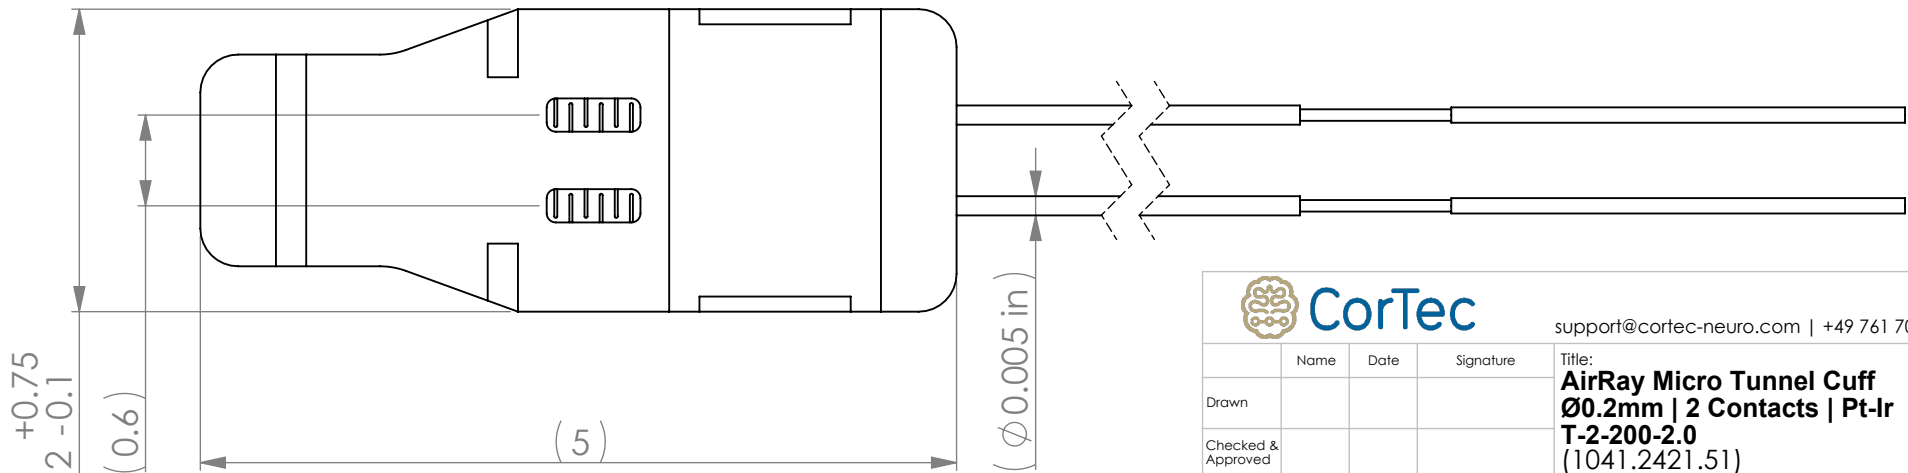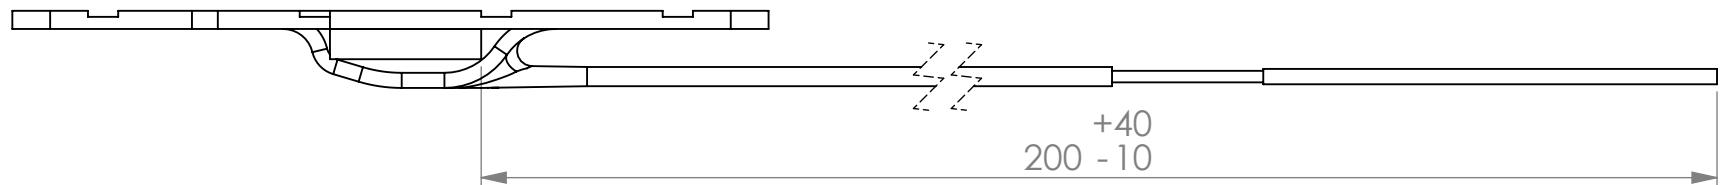

DRAWN FLAT FOR ILLUSTRATION PURPOSES ONLY

			support@cortec-neuro.com +49 761 70888100		
			Title: AirRay Micro Tunnel Cuff Ø0.2mm 2 Contacts Pt-Ir T-2-200-2.0 (1041.2421.51)		
Drawn	Name	Date	Signature	Drawing number:	Rev.:
Checked & Approved					
Changes:			FIRST ANGLE PROJECTION		
			Unit: mm	Material:	SCALE: 20:1
Replaces: -			Tolerance: ISO 2768-mK if not stated otherwise		SHEET 1 OF 1

This document is confidential. It contains designs and /or information that belongs to CorTec GmbH.
 This document may not, in whole or part, be duplicated or shared or disclosed or used for the manufacture of any part(s) herein,
 or for any other purpose, without the prior permission of CorTec GmbH.